

CO00001_26031804_ANALYZE_STANDARD_AND_SAMPLE_ FOR_B4502842 - CETIRIZINE HCL_20260318_202456

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

STANDARD ANALYSIS

Injection Data (Standard)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	928.551	4.45082	1.47511	81.071

No RSD data available for STANDARD.

STANDARD CHECKER ANALYSIS

Injection Data (Standard Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	682.453	4.06842	1.49191	67.327

SAMPLE ANALYSIS

Injection Data (Sample)

Order Number	Sample ID	Vial	Vessel	Revolver	Hole Revolver	Injection Number	Area	Retention Time (min)	Tailing Factor	Peak Height	Result of Equation
4	TE00003-1	5	1	1	1	1	819.634	4.19135	1.4746	72.764	None
5	TE00003-2	6	2	2	1	1	798.958	3.9491	1.4564	78.755	None
6	TE00003-3	7	3	3	1	1	846.89	3.9371	1.47006	83.036	None
7	TE00003-4	8	1	1	2	1	587.508	3.99865	1.50157	54.59	None
8	TE00003-5	9	2	2	2	1	941.081	3.98118	1.56347	86.351	None
9	TE00003-6	10	3	3	2	1	902.214	3.9841	1.54864	82.727	None

RSD Results (Sample)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
816.047	4.00691	123.729	0.0932567	15.162	2.3274

BASELINE ANALYSIS

Injection Data (Baseline)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	151.502	2.41708	0.652473	13.429
1	2	1	TE00001-1	9.4574	1.90698	0.952943	2.318
1	2	1	TE00001-1	4.97461	5.97232	0.527489	0.575
1	2	1	TE00001-1	1.49383	4.09015	0.528029	0.346
1	2	1	TE00001-1	0.131838	0.4956	0.546231	0.074

DETECTOR CHECKER ANALYSIS


Injection Data (Detector Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	857.893	3.9885	1.54655	78.798

IMAGE STANDARD

Image STANDARD for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202603\2_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_152133.txt

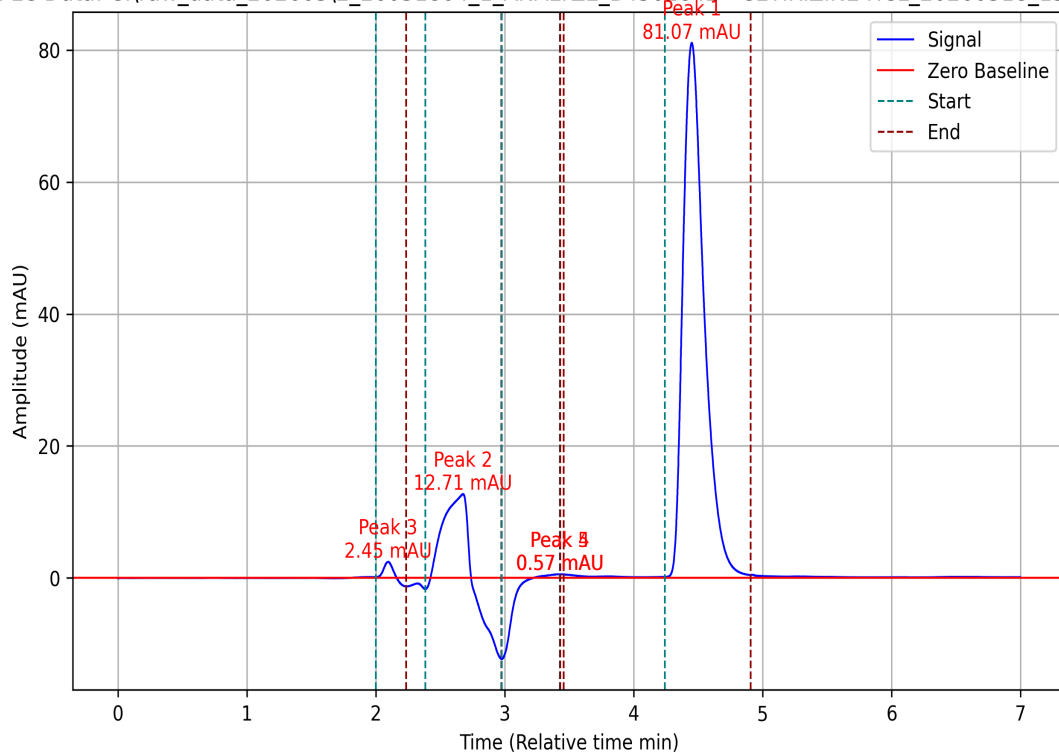

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	928.551	4.45082	1.47511	81.071

IMAGE DATA FOR STANDARD CHECKER

Image STANDARD CHECKER for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202603\3_26031804_1_STANDARD CHECKER_B4502842 - CETIRIZINE HCL_20260318_153315.txt

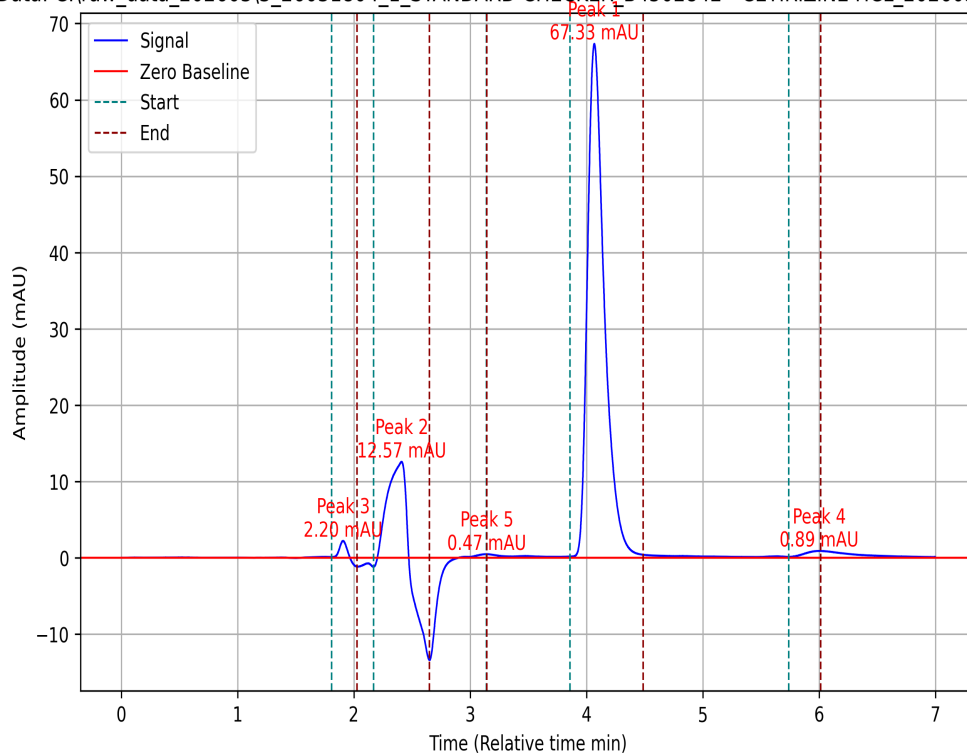

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	682.453	4.06842	1.49191	67.327

IMAGE DATA FOR SAMPLE

Image for SAMPLE Inject ID: TE00003-1
SAMPLE : 1

HPLC Data: C:\raw_data_202603\4_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_170301.txt

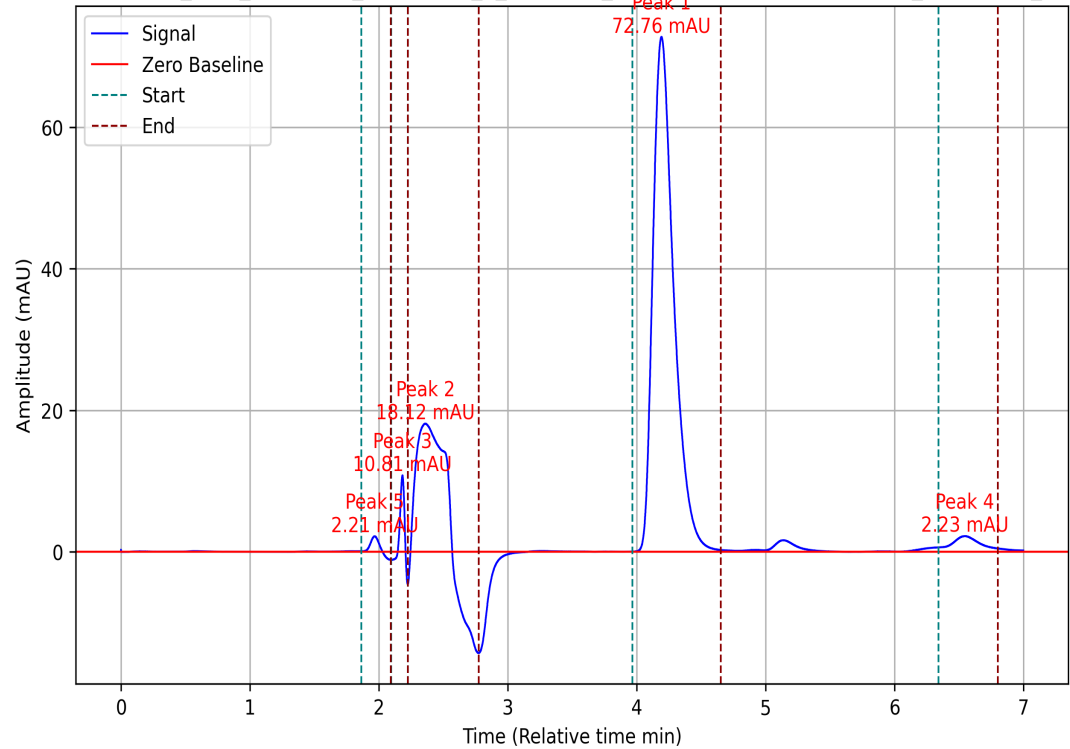


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volve r	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak He ight	Result of Equat ion
4	TE00003 -1	5	1	1	1	1	819.634	4.19135	1.4746	72.764	None

Image for SAMPLE Inject ID: TE00003-2
SAMPLE : 2

HPLC Data: C:\raw_data_202603\5_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_173349.txt

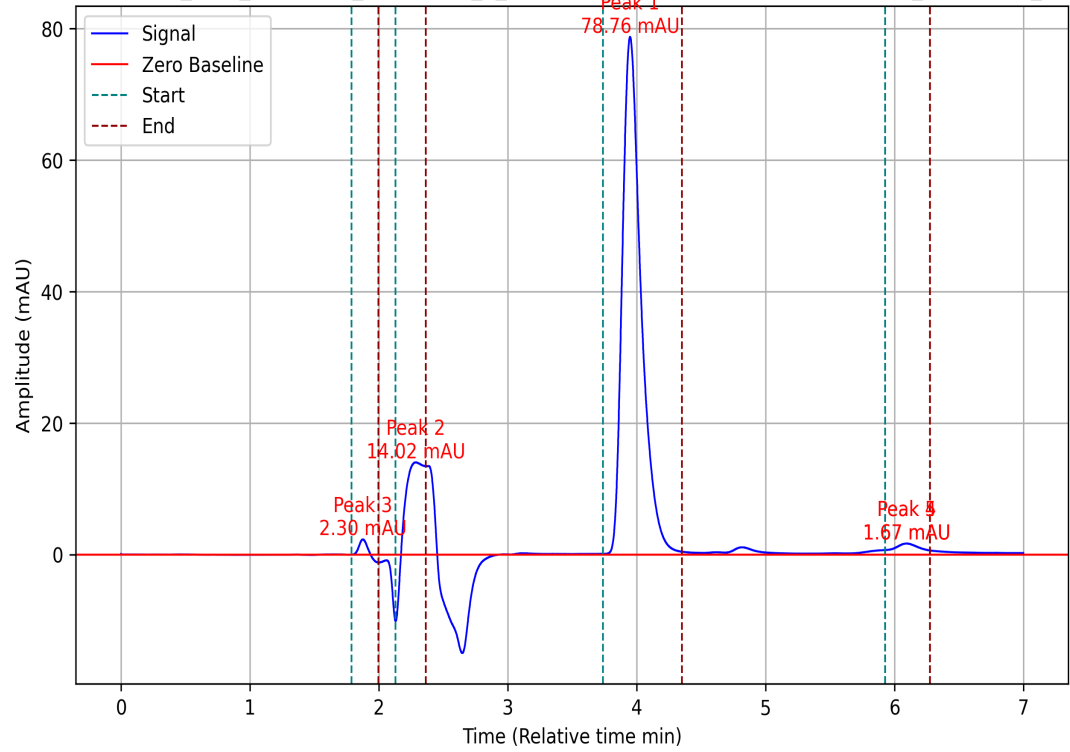


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
5	TE00003-2	6	2	2	1	1	798.958	3.9491	1.4564	78.755	None

Image for SAMPLE Inject ID: TE00003-3
SAMPLE : 3

HPLC Data: C:\raw_data_202603\6_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_181026.txt

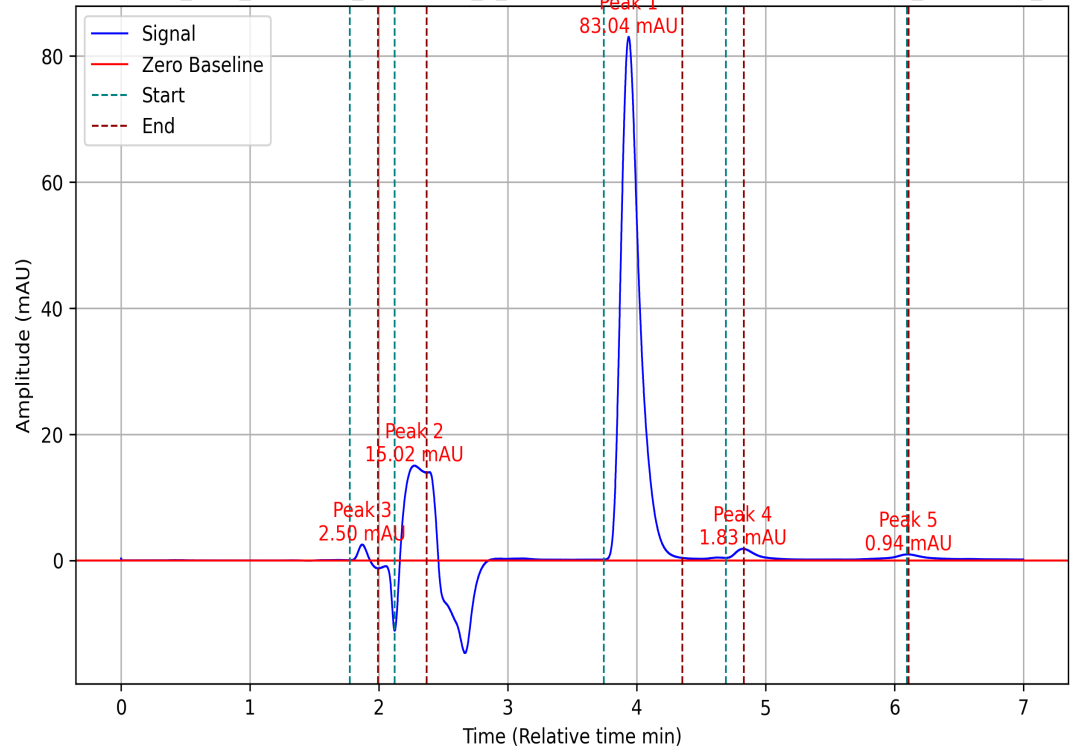


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
6	TE00003-3	7	3	3	1	1	846.89	3.9371	1.47006	83.036	None

Image for SAMPLE Inject ID: TE00003-4
SAMPLE : 4

HPLC Data: C:\raw_data_202603\7_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_185943.txt

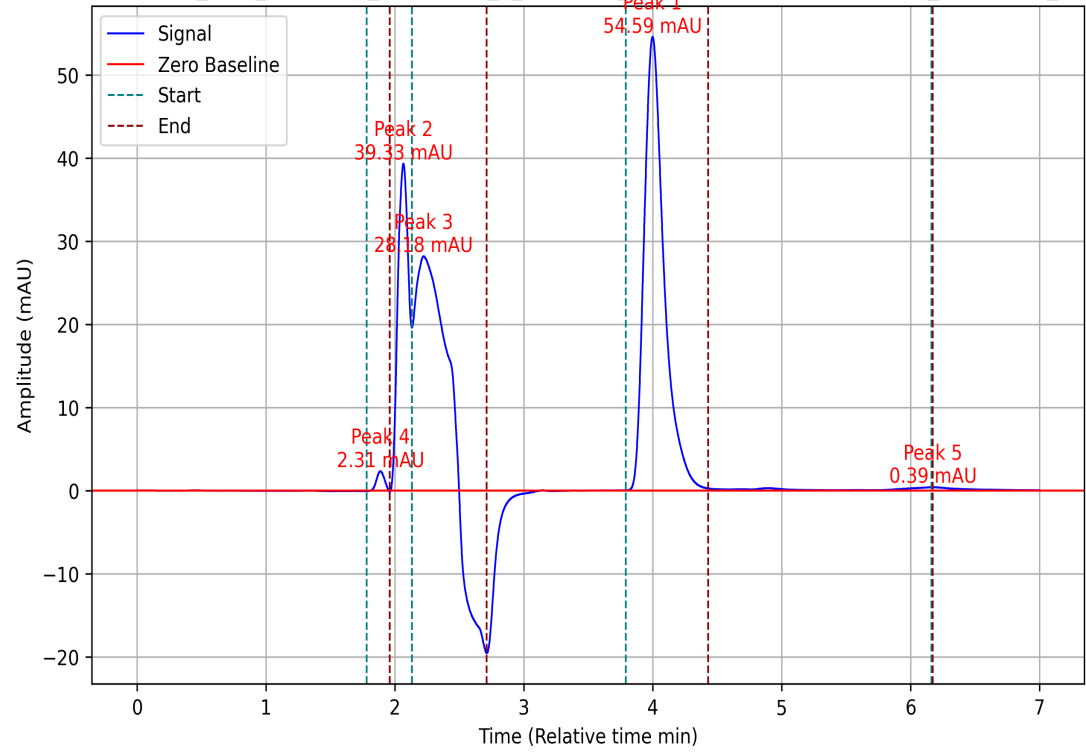


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
7	TE00003-4	8	1	1	2	1	587.508	3.99865	1.50157	54.59	None

Image for SAMPLE Inject ID: TE00003-5
SAMPLE : 5

HPLC Data: C:\raw_data_202603\8_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_192851.txt

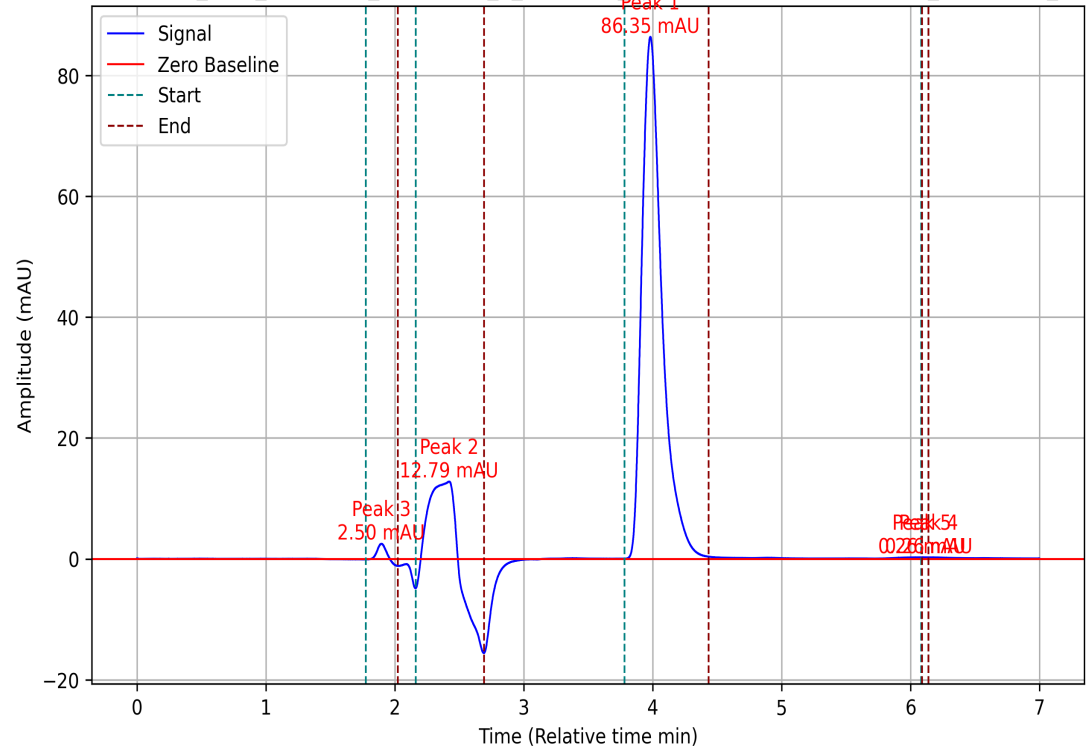


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
8	TE00003-5	9	2	2	2	1	941.081	3.98118	1.56347	86.351	None

Image for SAMPLE Inject ID: TE00003-6
SAMPLE : 6

HPLC Data: C:\raw_data_202603\9_26031804_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260318_200600.txt

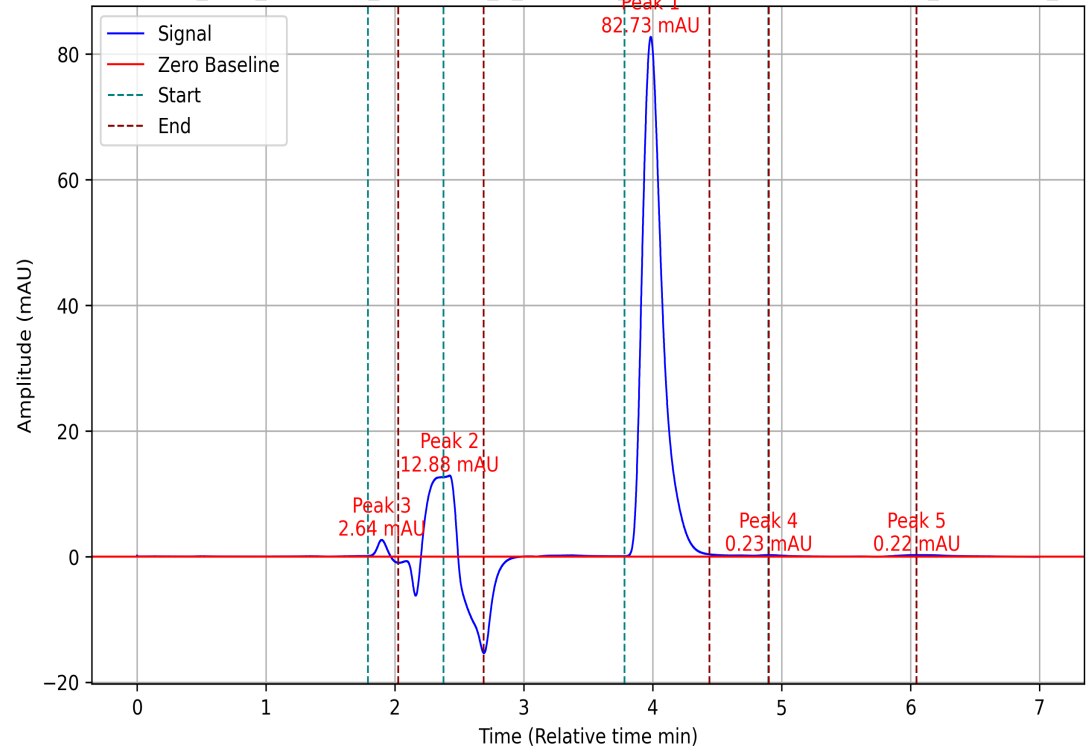

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
9	TE00003-6	10	3	3	2	1	902.214	3.9841	1.54864	82.727	None

IMAGE DATA FOR BASELINE

Image for BASELINE Inject ID: TE00001-1

HPLC Data: C:\raw_data_202603\1_26031804_1_CLEANSE CHECKER_B4502842 - CETIRIZINE HCL_20260318_150947.txt

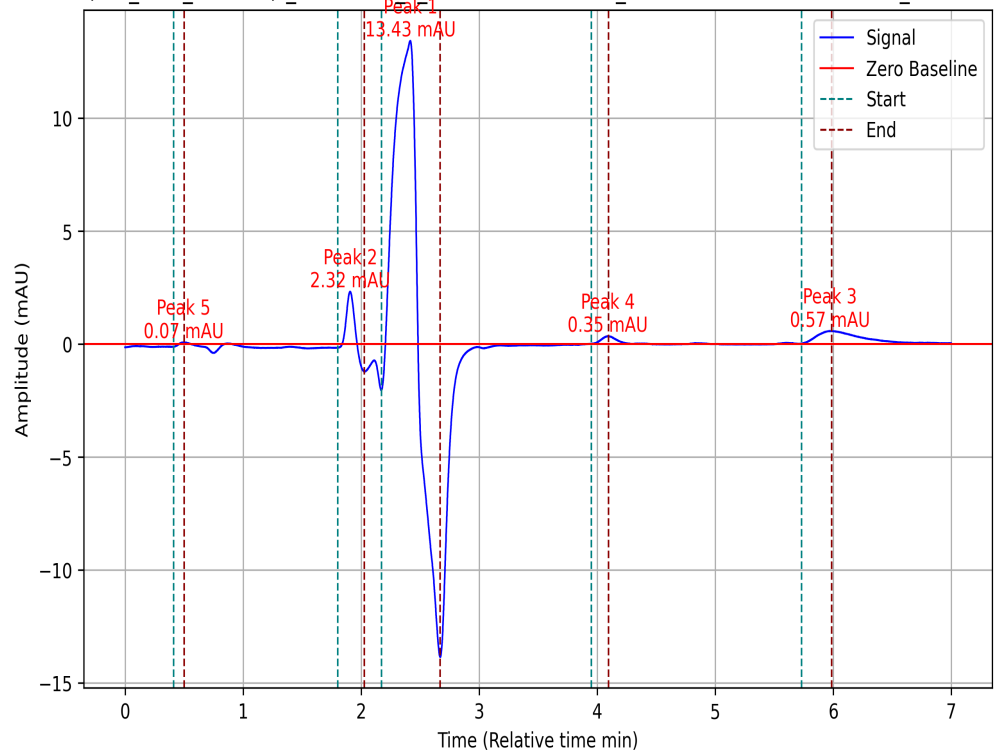


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	151.502	2.41708	0.652473	13.429
1	2	1	TE00001-1	9.4574	1.90698	0.952943	2.318
1	2	1	TE00001-1	4.97461	5.97232	0.527489	0.575
1	2	1	TE00001-1	1.49383	4.09015	0.528029	0.346
1	2	1	TE00001-1	0.131838	0.4956	0.546231	0.074

Image for DETECTOR CHECKER Inject ID: TE00002-2

HPLC Data: C:\raw_data_202603\10_26031804_1_DETECTOR CHECKER_B4502842 - CETIRIZINE HCL_20260318_201751.txt

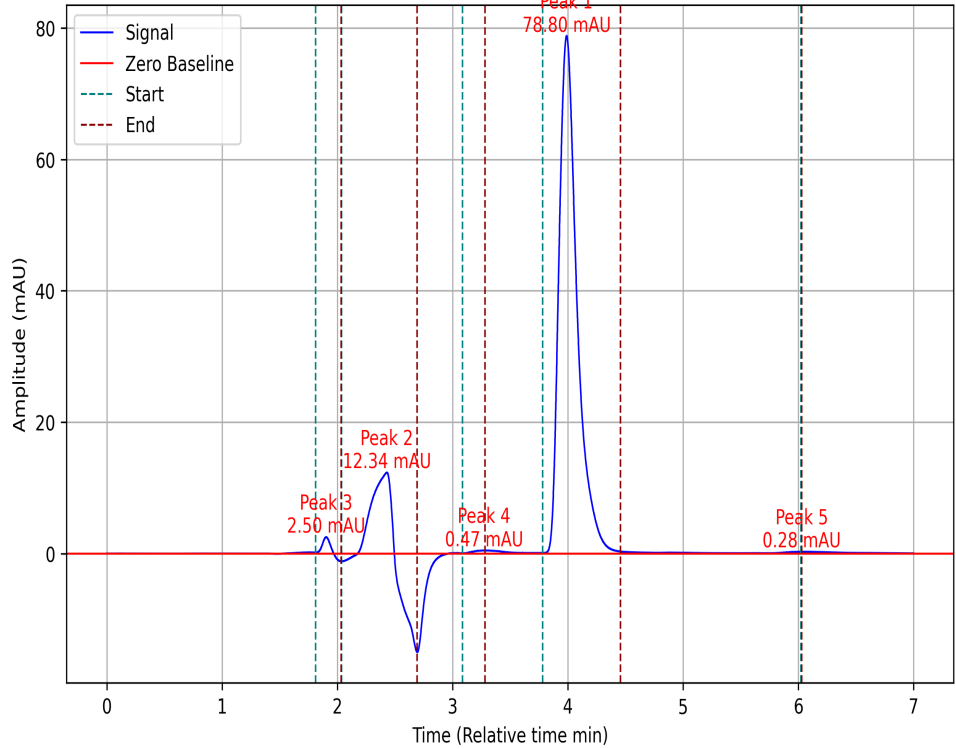

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26031804
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	857.893	3.9885	1.54655	78.798
10	4	1	TE00002-2	139.192	2.42892	0.636328	12.339
10	4	1	TE00002-2	11.4202	1.90292	0.840196	2.504
10	4	1	TE00002-2	3.39755	3.27333	0.524128	0.472
10	4	1	TE00002-2	0.092826	6.0293	0.5	0.284