

CO00001_26040901_ANALYZE_STANDARD_AND_SAMPLE_ FOR_B4502842 - CETIRIZINE HCL_20260409_223357

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

STANDARD ANALYSIS

Injection Data (Standard)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	854.071	3.83433	1.76473	76.745
2	3	2	TE00002-1	724.396	3.83562	1.80845	66.896
2	3	3	TE00002-1	774.044	3.82713	1.87962	70.934

RSD Results (Standard)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
784.17	3.83236	65.4279	0.00457501	8.34358	0.119378

STANDARD CHECKER ANALYSIS

Injection Data (Standard Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	825.954	3.81508	1.80335	75.531

SAMPLE ANALYSIS

Injection Data (Sample)

Order Number	Sample ID	Vial	Vessel	Revolver	Hole Revolver	Injection Number	Area	Retention Time (min)	Tailing Factor	Peak Height	Result of Equation
4	TE00003-1	5	1	1	1	1	817.037	3.81408	1.8473	74.594	None
5	TE00003-2	6	2	2	1	1	877.05	3.80417	1.81289	80.498	None

RSD Results (Sample)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
847.044	3.80912	42.4356	0.00700743	5.00985	0.183964

BASELINE ANALYSIS

Injection Data (Baseline)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	176.421	2.50012	0.766528	13.512
1	2	1	TE00001-1	9.43884	1.97932	0.812225	2.118
1	2	1	TE00001-1	1.44774	0.30725	0.528791	0.444
1	2	1	TE00001-1	0.101585	6.19007	0.5	0.316

DETECTOR CHECKER ANALYSIS


Injection Data (Detector Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	835.499	3.83398	1.84546	77.474

IMAGE STANDARD

Image STANDARD for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202604\2_26040901_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260409_191928.txt

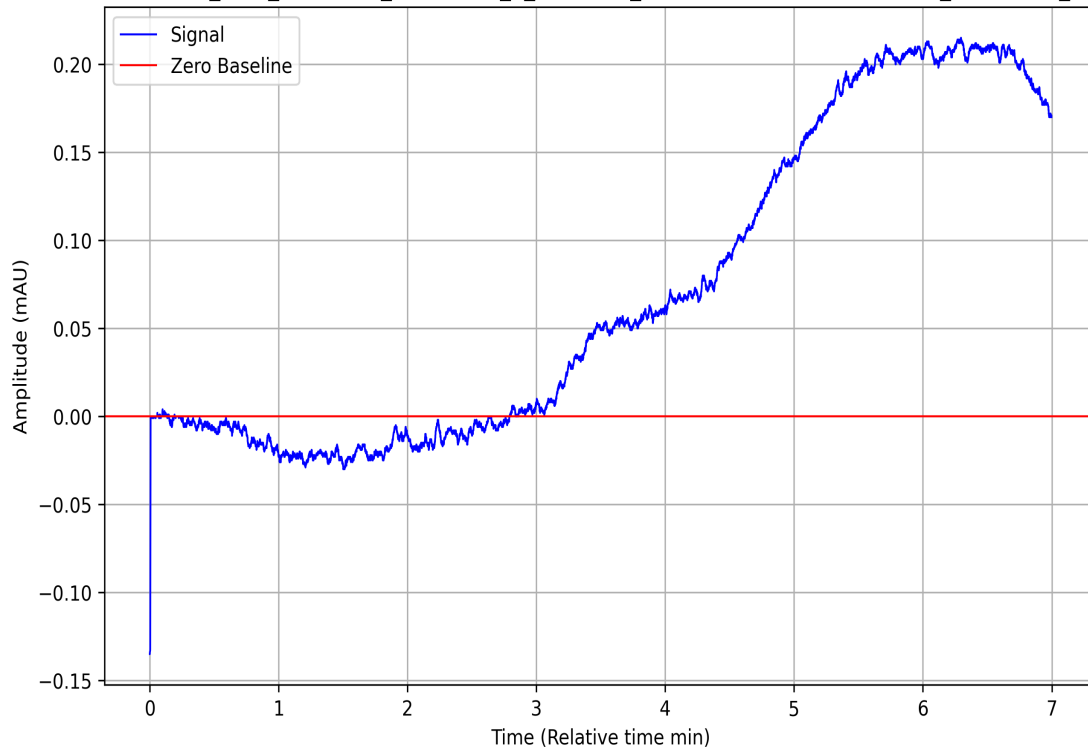


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	854.071	3.83433	1.76473	76.745

Image STANDARD for Inject ID: TE00002-1

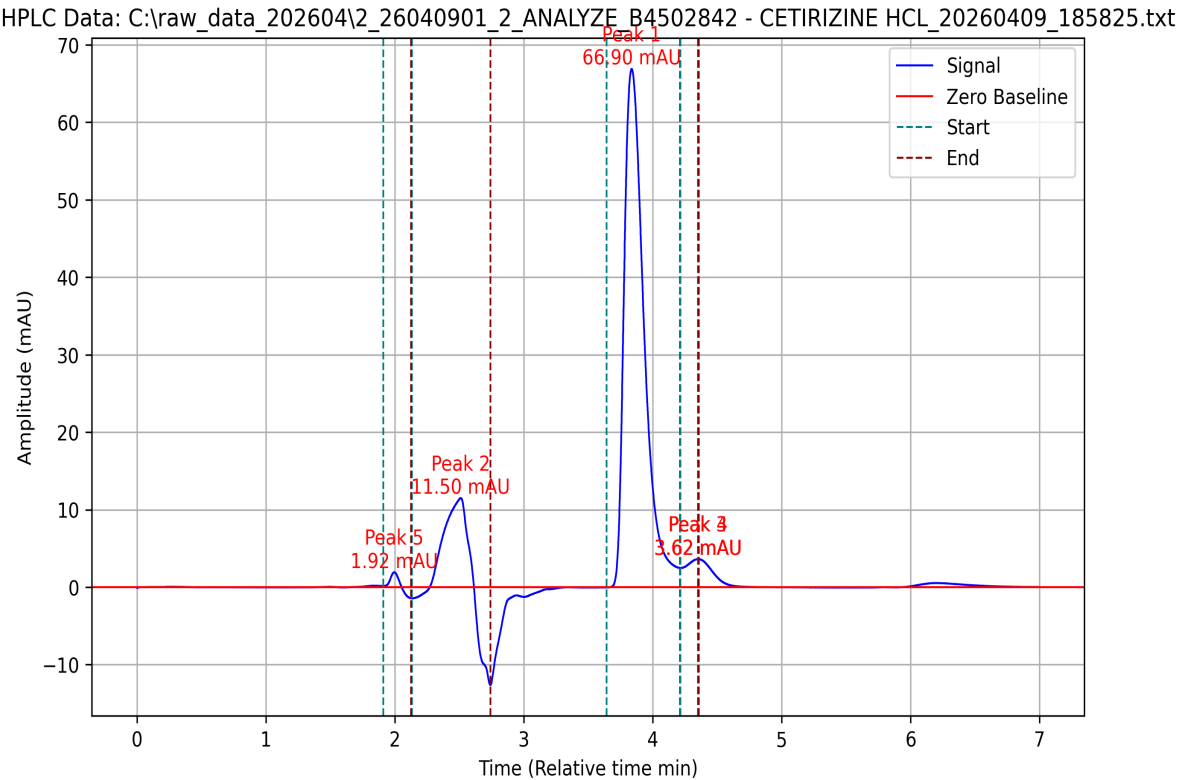


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	2	TE00002-1	724.396	3.83562	1.80845	66.896

Image STANDARD for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202604\2_26040901_3_ANALYZE_B4502842 - CETIRIZINE HCL_20260409_193153.txt

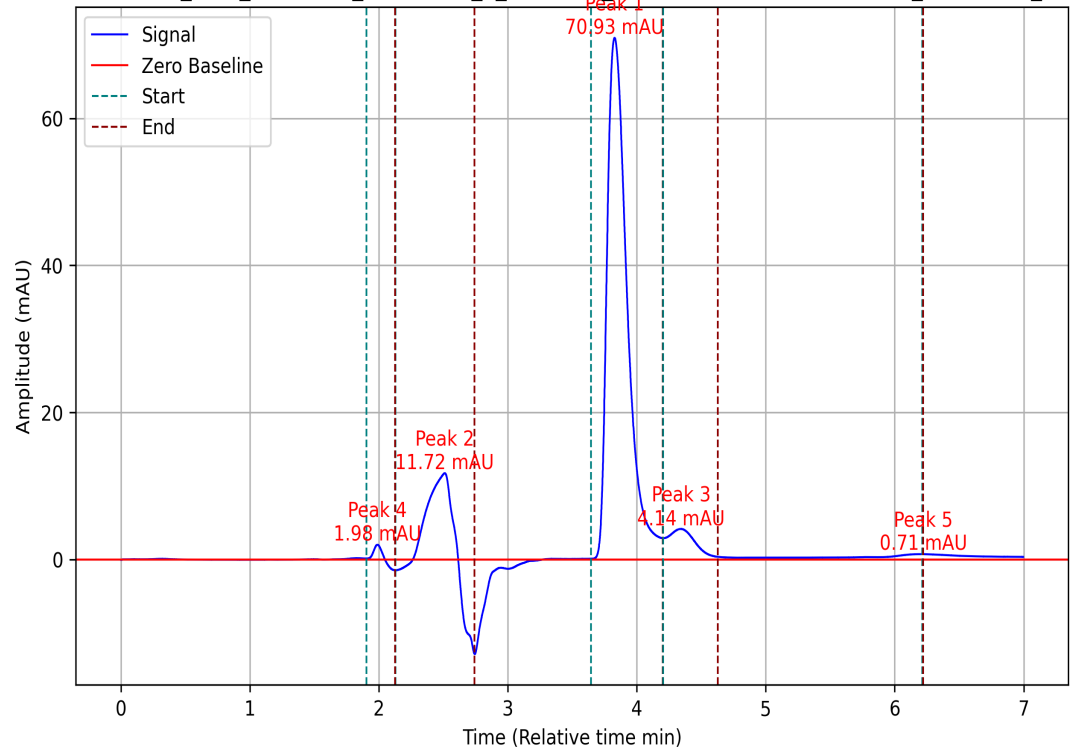

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	3	TE00002-1	774.044	3.82713	1.87962	70.934

IMAGE DATA FOR STANDARD CHECKER

Image STANDARD CHECKER for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202604\3_26040901_1_STANDARD CHECKER_B4502842 - CETIRIZINE HCL_20260409_194710.txt

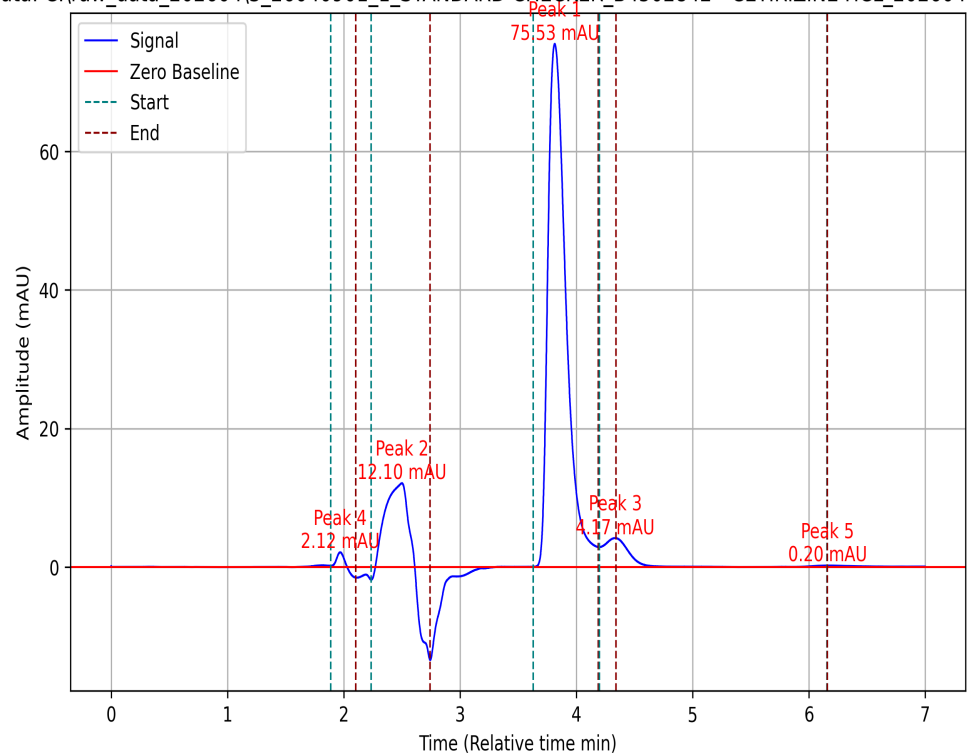

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	825.954	3.81508	1.80335	75.531

IMAGE DATA FOR SAMPLE

Image for SAMPLE Inject ID: TE00003-1
SAMPLE : 1

HPLC Data: C:\raw_data_202604\4_26040901_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260409_211003.txt

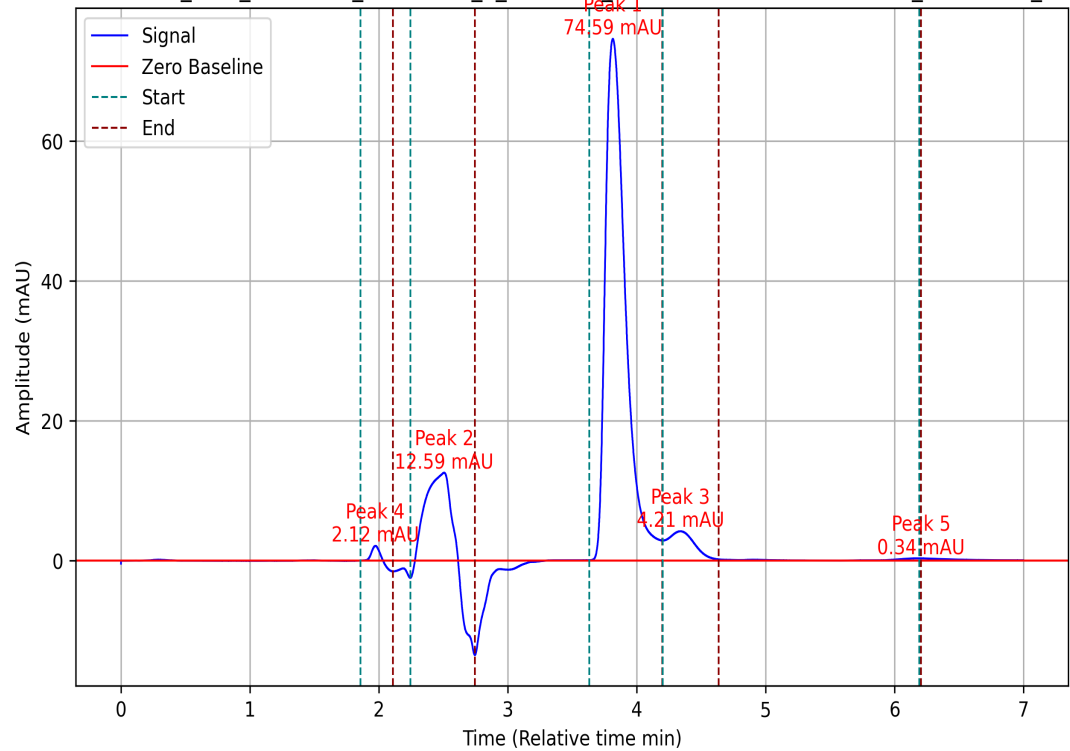


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
4	TE00003-1	5	1	1	1	1	817.037	3.81408	1.8473	74.594	None

Image for SAMPLE Inject ID: TE00003-2
SAMPLE : 2

HPLC Data: C:\raw_data_202604\5_26040901_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260409_215803.txt

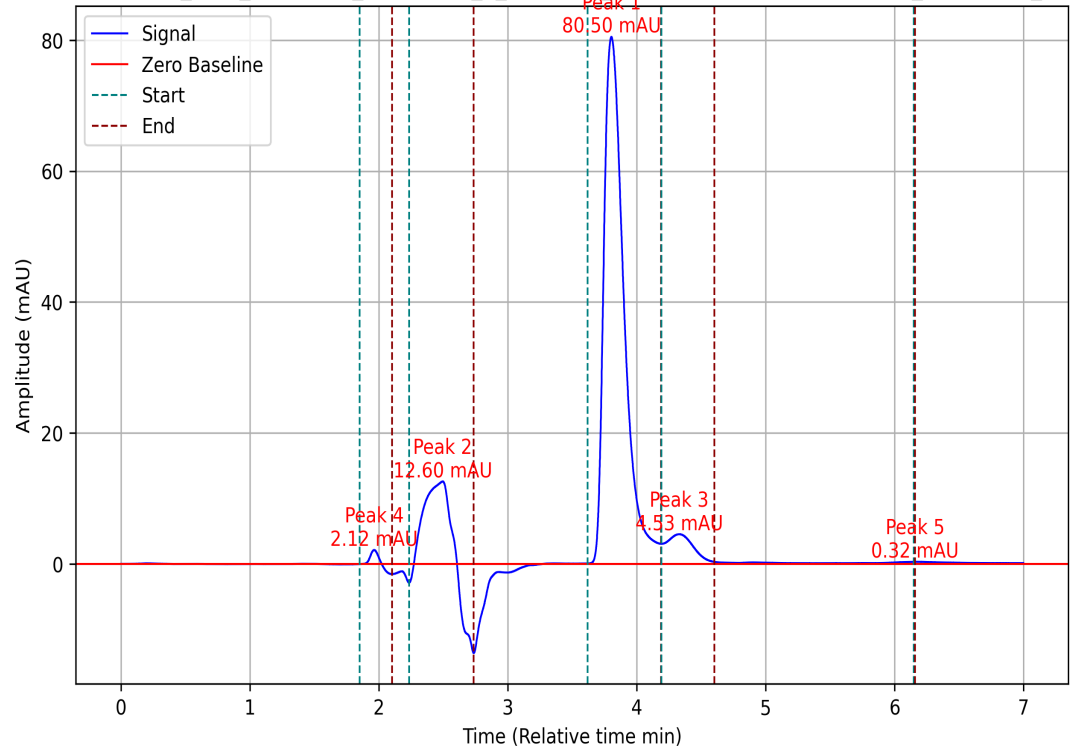

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
5	TE00003-2	6	2	2	1	1	877.05	3.80417	1.81289	80.498	None

IMAGE DATA FOR BASELINE

Image for BASELINE Inject ID: TE00001-1

HPLC Data: C:\raw_data_202604\1_26040901_1_CLEANSE CHECKER_B4502842 - CETIRIZINE HCL_20260409_181919.txt

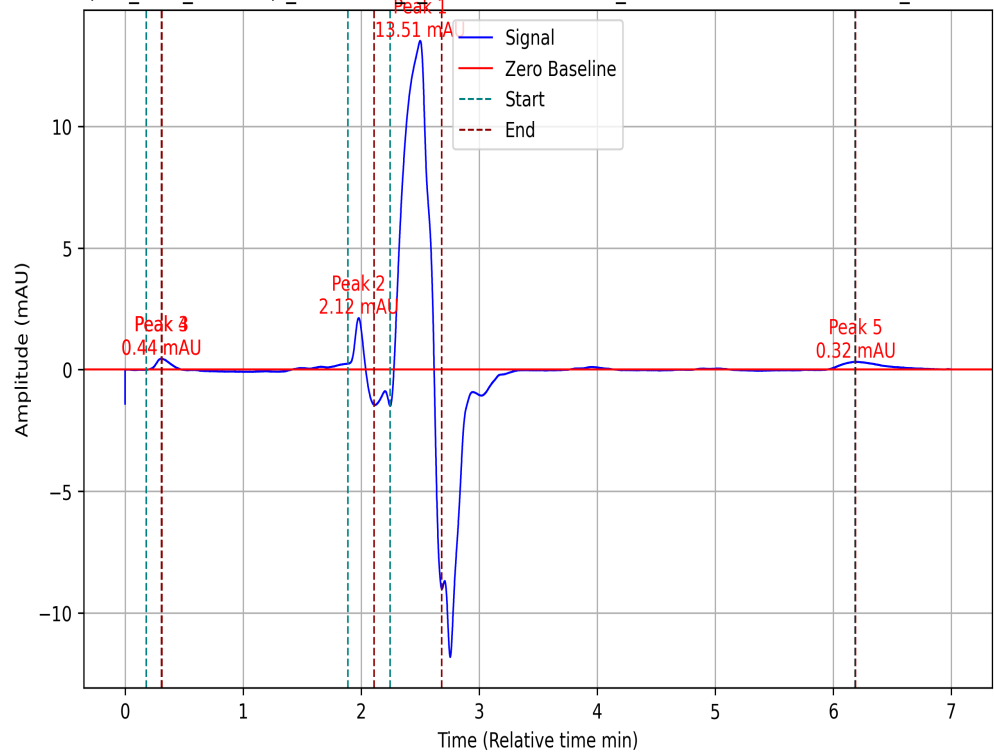


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	176.421	2.50012	0.766528	13.512
1	2	1	TE00001-1	9.43884	1.97932	0.812225	2.118
1	2	1	TE00001-1	1.44774	0.30725	0.528791	0.444
1	2	1	TE00001-1	0.101585	6.19007	0.5	0.316

Image for DETECTOR CHECKER Inject ID: TE00002-2

HPLC Data: C:\raw_data_202604\10_26040901_1_DETECTOR CHECKER_B4502842 - CETIRIZINE HCL_20260409_222654.txt

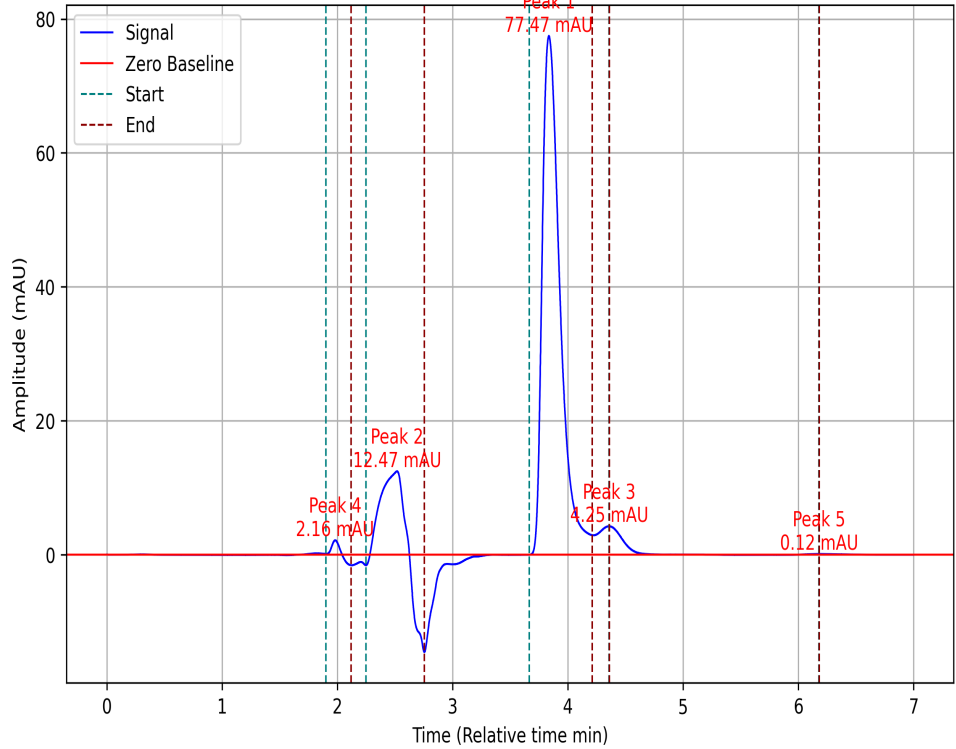

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26040901
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B858A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	835.499	3.83398	1.84546	77.474
10	4	1	TE00002-2	165.394	2.51835	0.725604	12.466
10	4	1	TE00002-2	0.429098	4.35957	0.5	4.249
10	4	1	TE00002-2	9.11901	1.98025	0.86309	2.156
10	4	1	TE00002-2	0.0245225	6.18023	0.5	0.115