

CO00001_26030402_ANALYZE_STANDARD_AND_SAMPLE_ FOR_B4502842 - CETIRIZINE HCL_20260312_145937

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

STANDARD ANALYSIS

Injection Data (Standard)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	870.611	3.66358	1.57785	104.951

No RSD data available for STANDARD.

STANDARD CHECKER ANALYSIS

Injection Data (Standard Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	869.557	3.64722	1.61587	105.279

SAMPLE ANALYSIS

Injection Data (Sample)

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak He ight	Result of Equat ion
4	TE00003 -1	5	1	1	1	1	788.112	3.62147	1.58074	98.106	None
5	TE00003 -2	6	2	2	1	1	796.544	3.62143	1.57985	100.886	None
6	TE00003 -3	7	3	3	1	1	1017.55	4.97763	1.6054	126.31	None

RSD Results (Sample)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
867.402	4.07351	130.1	0.782991	14.9988	19.2215

BASELINE ANALYSIS

Injection Data (Baseline)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	156.942	2.48015	0.851942	14.366
1	2	1	TE00001-1	7.76304	2.02147	1.04152	2.158


DETECTOR CHECKER ANALYSIS

No Injection data available for DETECTOR CHECKER.

IMAGE STANDARD

Image STANDARD for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202603\2_26030402_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260304_180456.txt

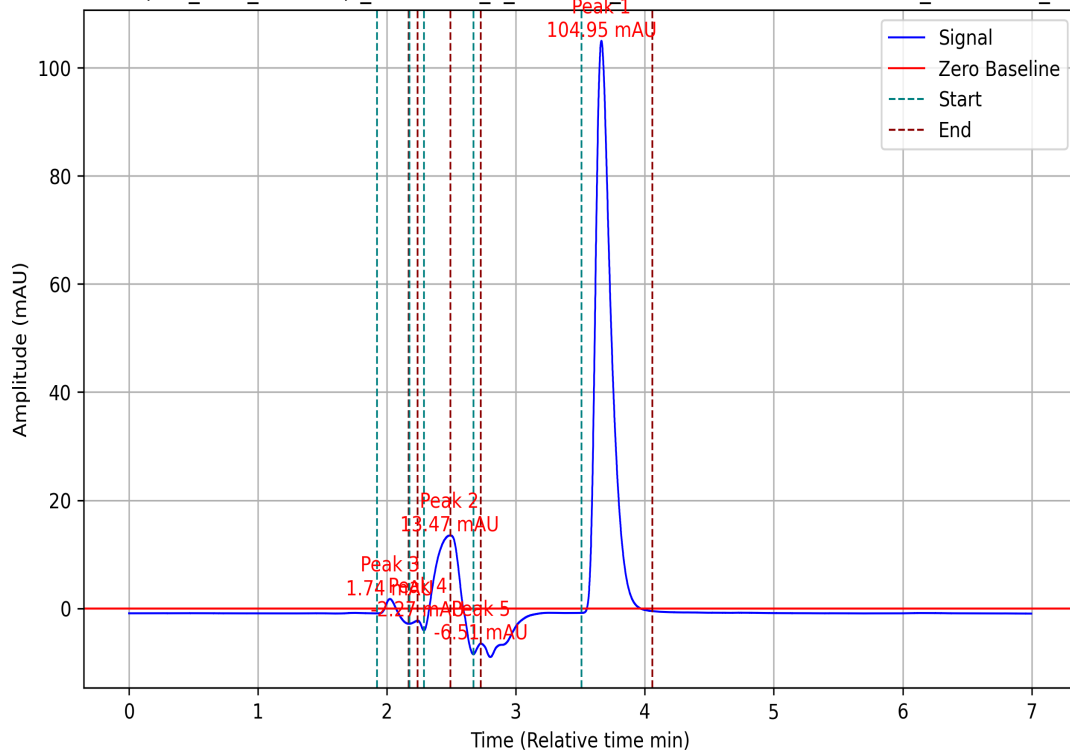

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	1	TE00002-1	870.611	3.66358	1.57785	104.951

IMAGE DATA FOR STANDARD CHECKER

Image STANDARD CHECKER for Inject ID: TE00002-1

HPLC Data: C:\raw_data_202603\3_26030402_1_STANDARD CHECKER_B4502842 - CETIRIZINE HCL_20260304_181642.txt

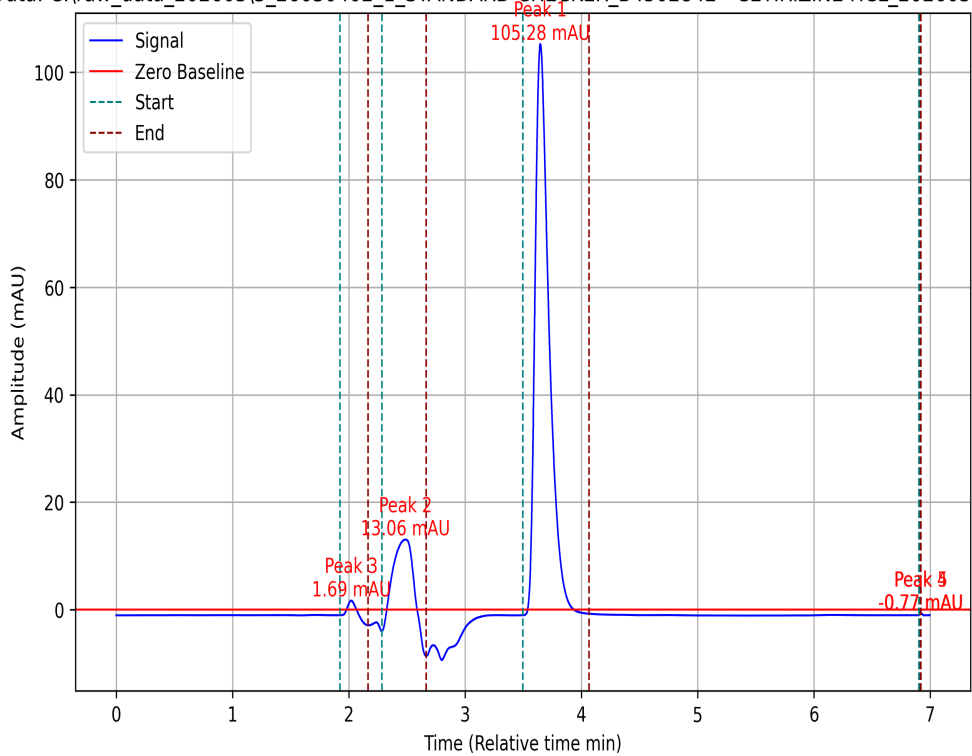

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	869.557	3.64722	1.61587	105.279

IMAGE DATA FOR SAMPLE

Image for SAMPLE Inject ID: TE00003-1
SAMPLE : 1

HPLC Data: C:\raw_data_202603\4_26030402_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260304_193524.txt

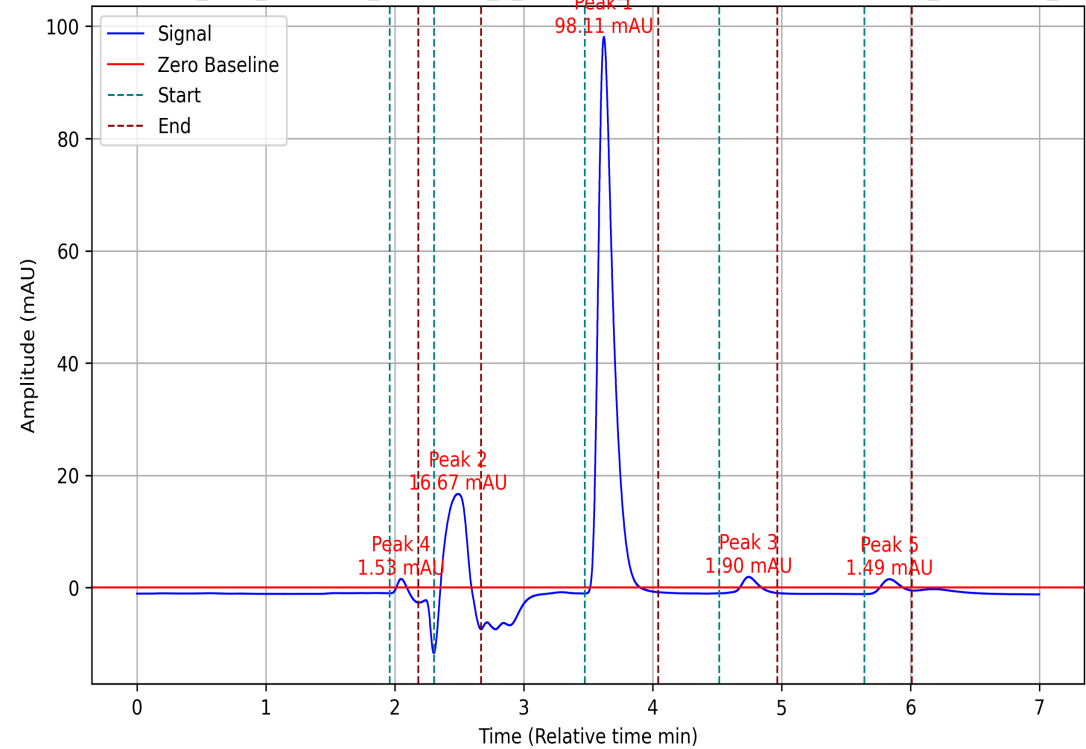


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volve r	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak He ight	Result of Equat ion
4	TE00003 -1	5	1	1	1	1	788.112	3.62147	1.58074	98.106	None

Image for SAMPLE Inject ID: TE00003-2
SAMPLE : 2

HPLC Data: C:\raw_data_202603\5_26030402_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260304_201346.txt

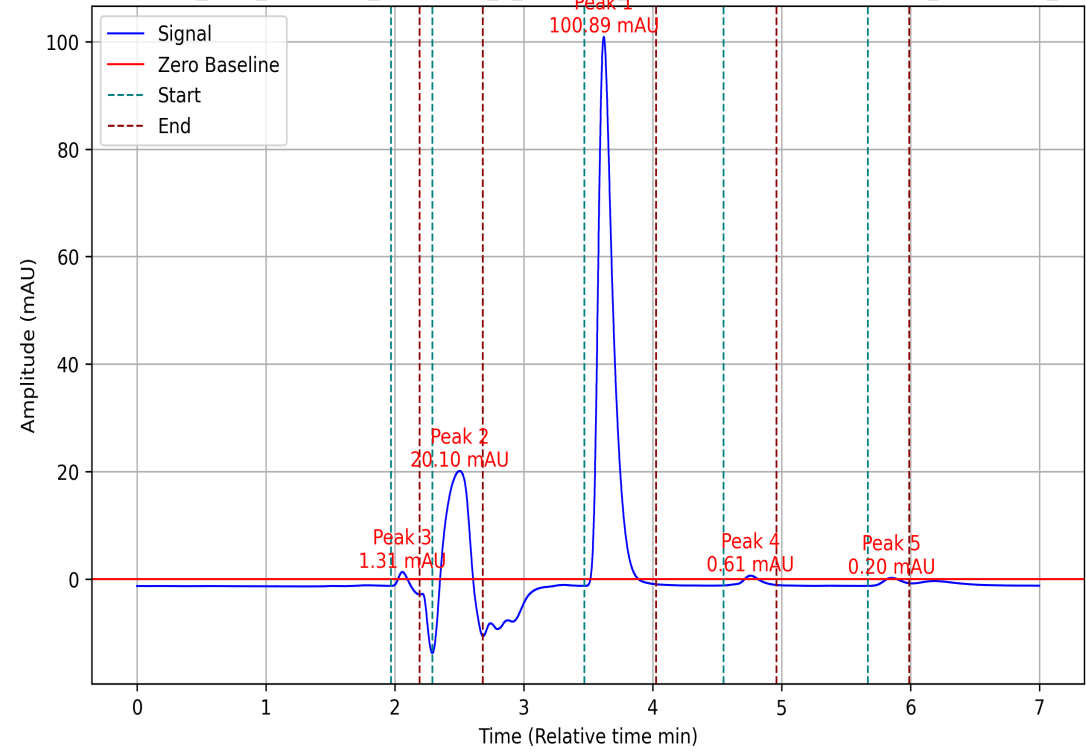


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
5	TE00003-2	6	2	2	1	1	796.544	3.62143	1.57985	100.886	None

Image for SAMPLE Inject ID: TE00003-3
SAMPLE : 3

HPLC Data: C:\raw_data_202603\6_26030402_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260304_203525.txt

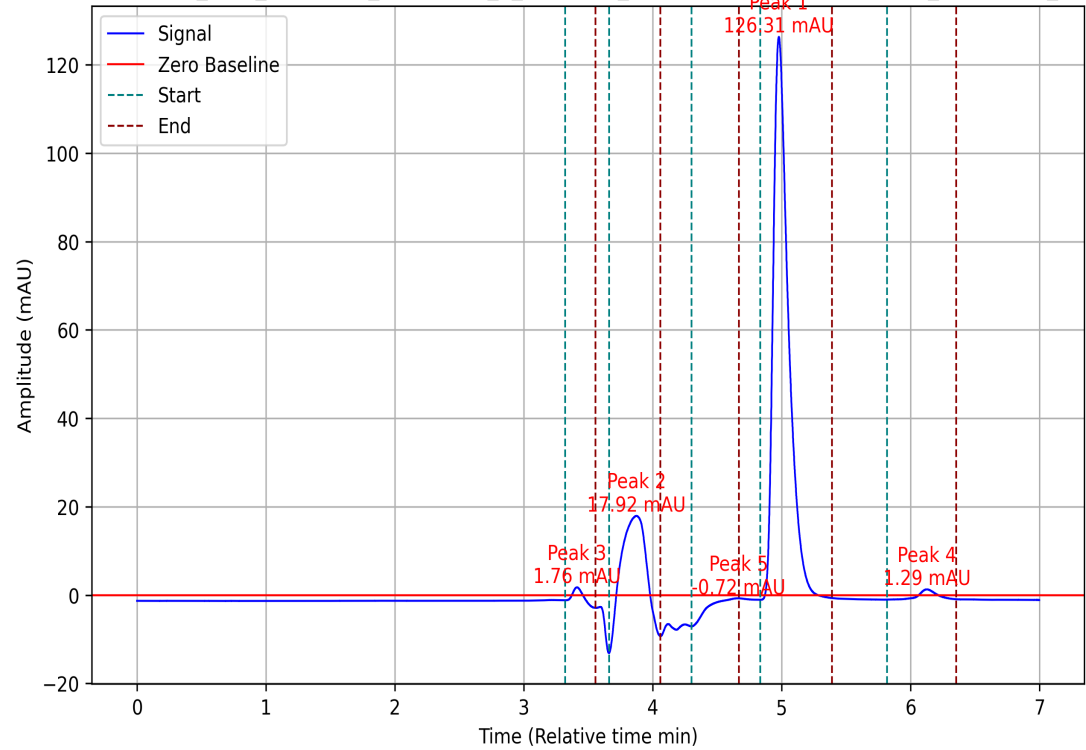

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Sample ID	Vial	Vessel	Revolve r	Hole Re volver	Injection Number	Area	Retentio n Time (min)	Tailing Factor	Peak Height	Result of Equat ion
6	TE00003-3	7	3	3	1	1	1017.55	4.97763	1.6054	126.31	None

IMAGE DATA FOR BASELINE

Image for BASELINE Inject ID: TE00001-1

HPLC Data: C:\raw_data_202603\1_26030402_1_CLEANSE CHECKER_B4502842 - CETIRIZINE HCL_20260304_175312.txt

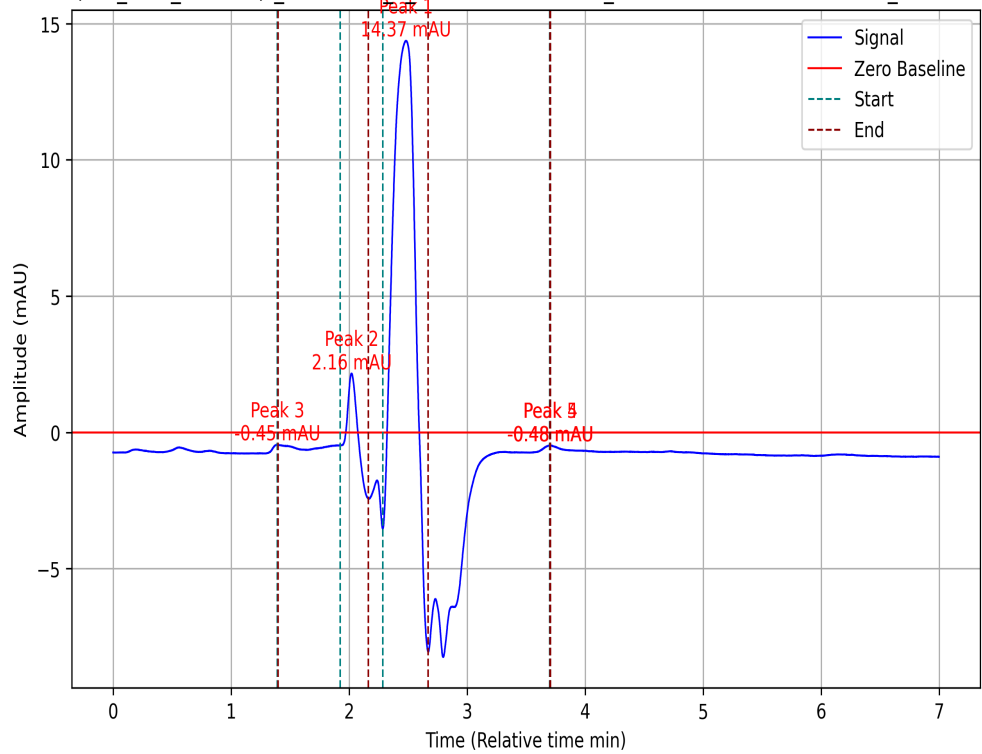

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26030402
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B523A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	156.942	2.48015	0.851942	14.366
1	2	1	TE00001-1	7.76304	2.02147	1.04152	2.158

IMAGE DATA FOR DETECTOR CHECKER

No images found for this analysis.