

CO00001_26022301_ANALYZE_STANDARD_AND_SAMPLE_ FOR_B4502842 - CETIRIZINE HCL_20260224_083625

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

STANDARD ANALYSIS

Injection Data (Standard)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	4	TE00002-1	1032.22	3.97633	1.59884	115.637
2	3	5	TE00002-1	1010.1	3.9665	1.57265	116.043

RSD Results (Standard)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
1021.16	3.97142	15.6412	0.00695086	1.53171	0.175022

STANDARD CHECKER ANALYSIS

Injection Data (Standard Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	775.019	3.96343	1.59408	90.025

SAMPLE ANALYSIS

Injection Data (Sample)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height	Result of Equation
4	5	1	TE00003-1	905.902	3.77065	1.59884	108.878	0.0
5	6	1	TE00003-2	576.515	3.72283	1.59898	71.028	0.0
6	7	1	TE00003-3	997.553	2.49867	1.05885	47.248	0.0
7	8	1	TE00003-4	955.592	2.51888	1.07231	45.055	0.0
8	9	1	TE00003-5	872.074	3.72732	1.58973	101.22	0.0
9	10	1	TE00003-6	1024.95	3.72893	1.57945	120.879	0.0

RSD Results (Sample)

Average Area	Average Retention Time (min)	Standard Deviation Area	Standard Deviation Retention Time	RSD Area (%)	RSD Retention Time (%)
888.764	3.32788	163.046	0.634743	18.3452	19.0735

BASELINE ANALYSIS

Injection Data (Baseline)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	237.645	2.46422	1.05396	16.025
1	2	1	TE00001-1	67.5037	4.95365	1.29104	5.783
1	2	1	TE00001-1	20.8548	1.99585	0.943122	3.498
1	2	1	TE00001-1	48.1471	6.2029	1.10672	3.06
1	2	1	TE00001-1	12.8517	3.95117	0.51616	2.153

DETECTOR CHECKER ANALYSIS


Injection Data (Detector Checker)

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	932.033	3.72928	1.5696	111.682
10	4	1	TE00002-2	191.306	2.59432	0.617663	13.235
10	4	1	TE00002-2	15.3047	2.03522	0.880759	2.976
10	4	1	TE00002-2	0.926144	4.23712	0.5	1.604
10	4	1	TE00002-2	0.095004	4.9826	0.5	0.915

IMAGE STANDARD

Image STANDARD for Inject ID: 4

HPLC Data: C:\raw_data_202602\2_26022301_4_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_164453.txt

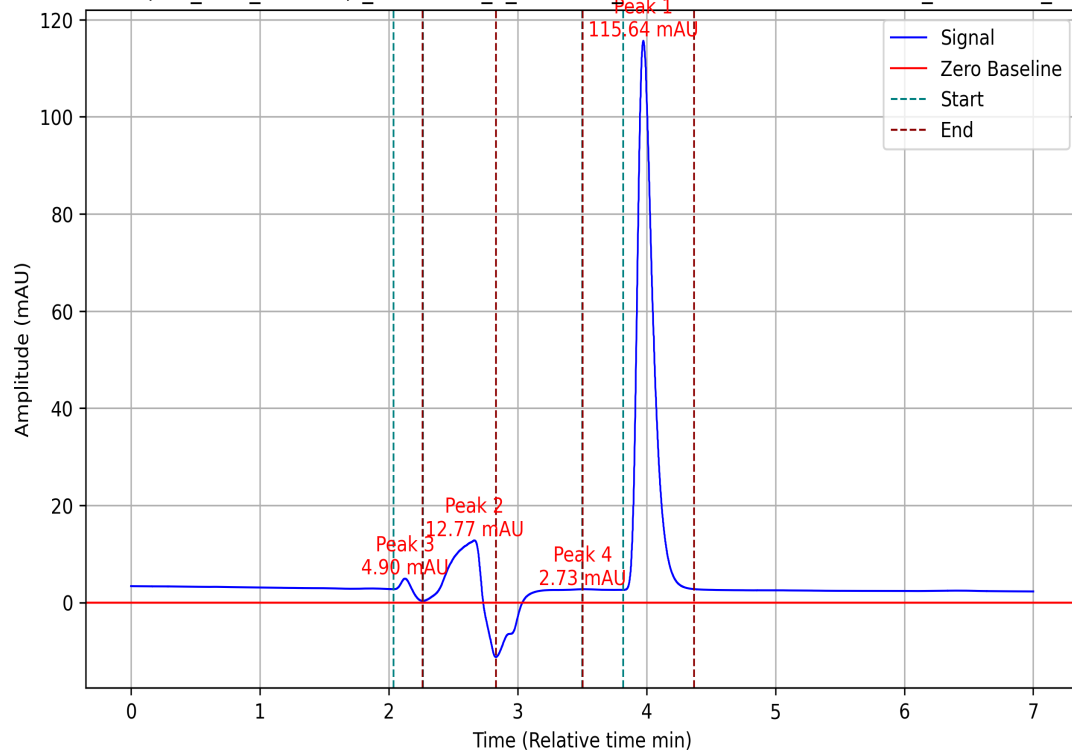


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	4	TE00002-1	1032.22	3.97633	1.59884	115.637

Image STANDARD for Inject ID: 5

HPLC Data: C:\raw_data_202602\2_26022301_5_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_165610.txt

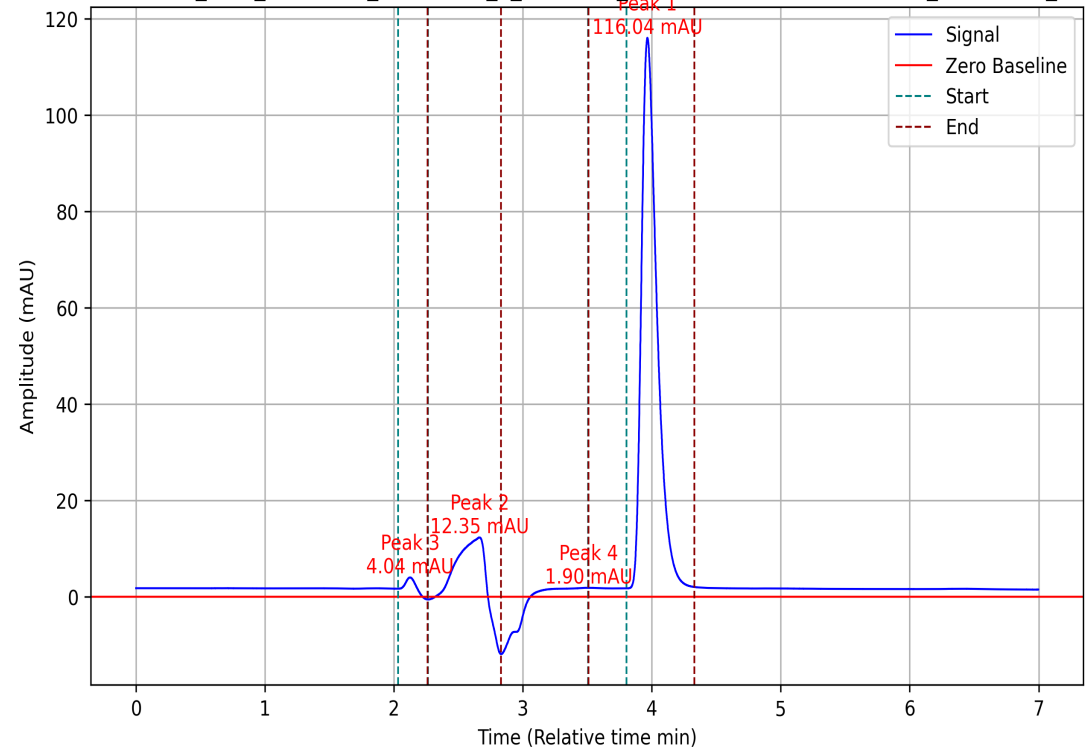

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
2	3	5	TE00002-1	1010.1	3.9665	1.57265	116.043

IMAGE DATA FOR STANDARD CHECKER

Image STANDARD CHECKER for Inject ID: 1

HPLC Data: C:\raw_data_202602\3_26022301_1_STANDARD CHECKER_B4502842 - CETIRIZINE HCL_20260223_170752.txt

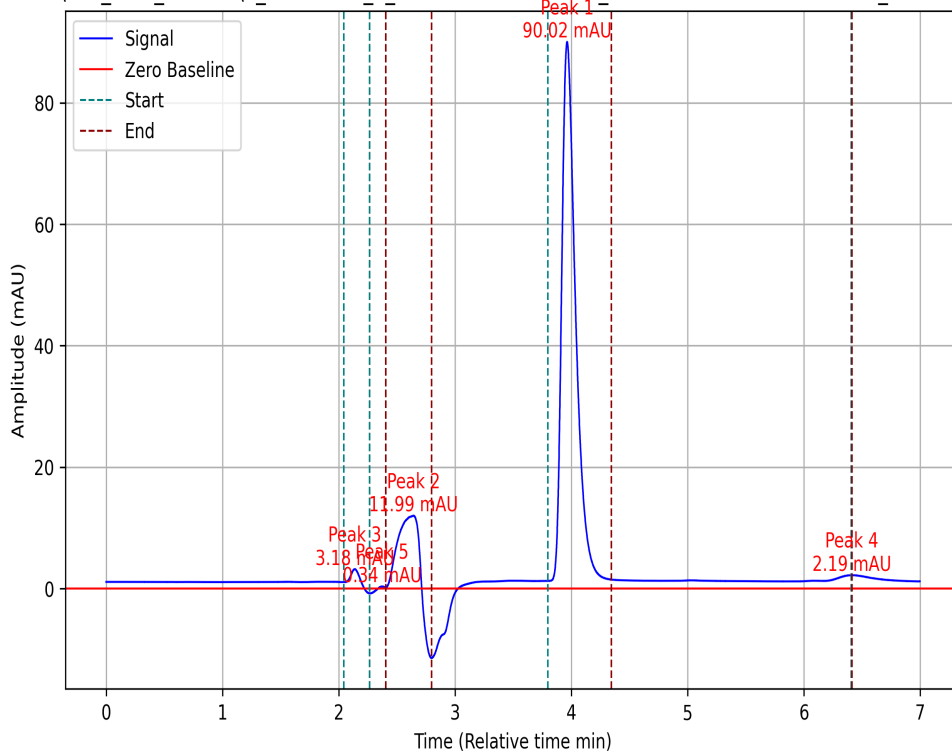

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
3	4	1	TE00002-2	775.019	3.96343	1.59408	90.025

IMAGE DATA FOR SAMPLE

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\4_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_183042.txt

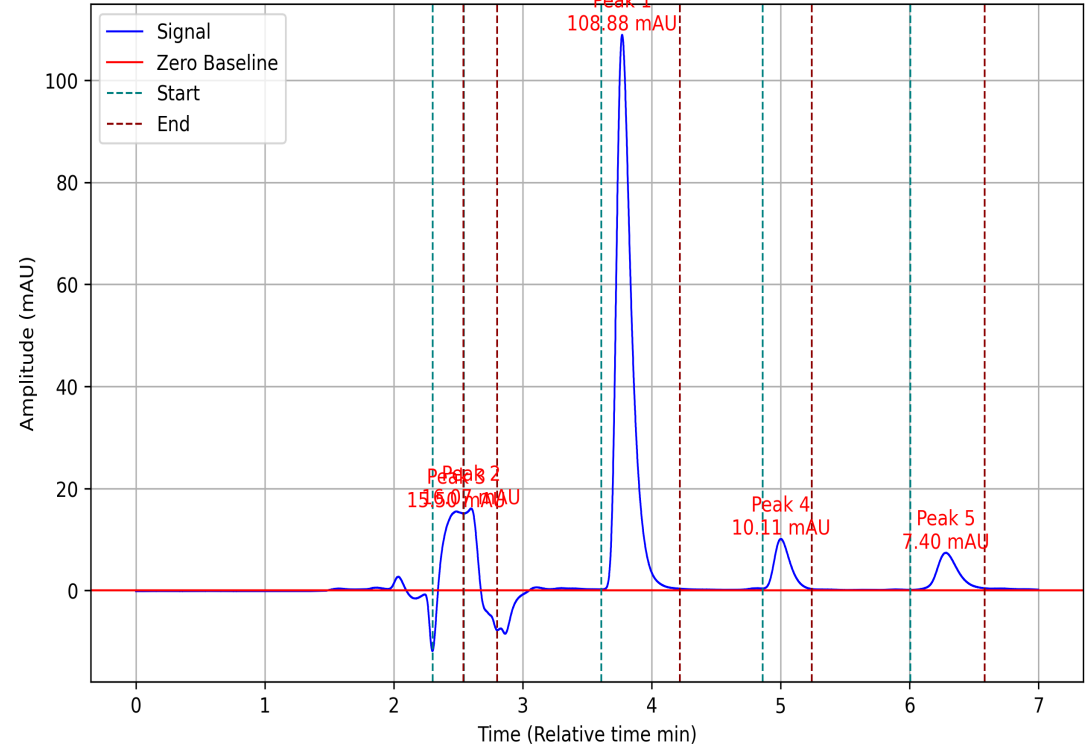


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
4	5	1	TE00003-1	905.902	3.77065	1.59884	108.878

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\5_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_190407.txt

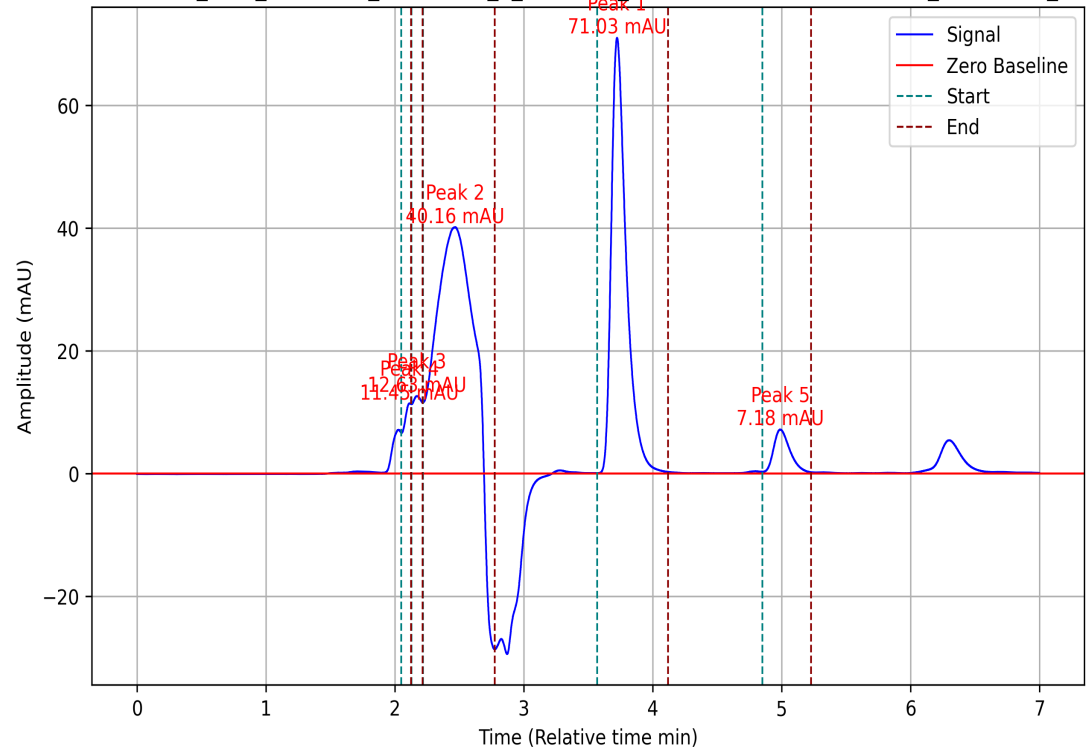


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
5	6	1	TE00003-2	576.515	3.72283	1.59898	71.028

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\6_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_194224.txt

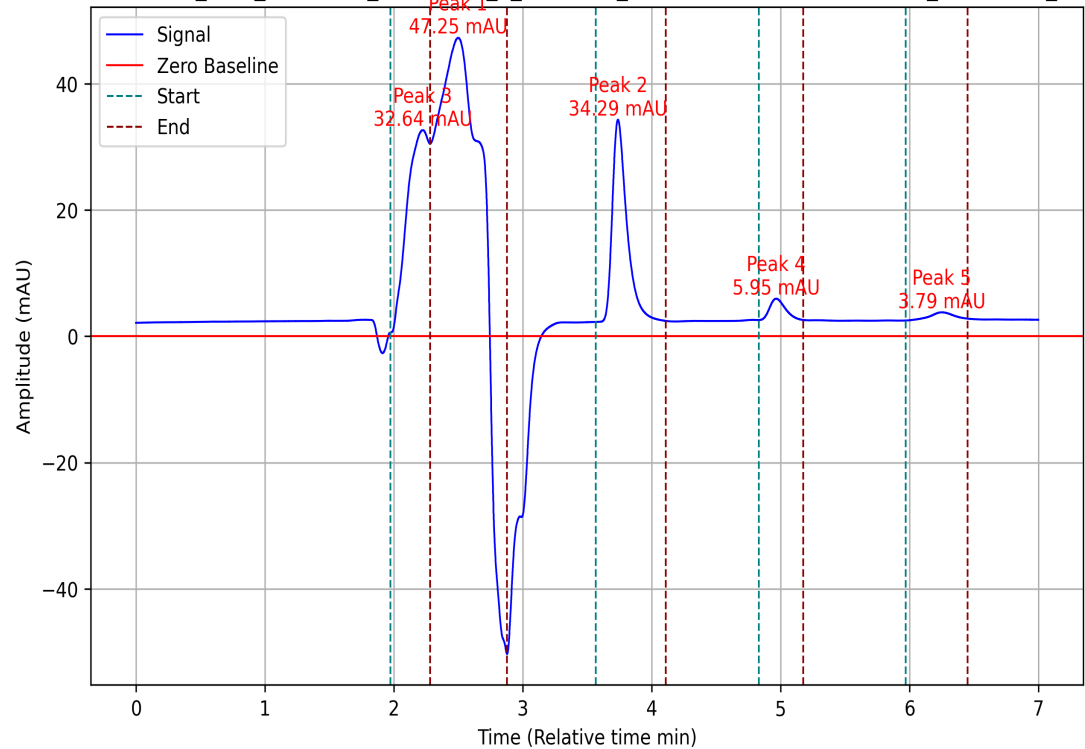


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
6	7	1	TE00003-3	997.553	2.49867	1.05885	47.248

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\7_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_201212.txt

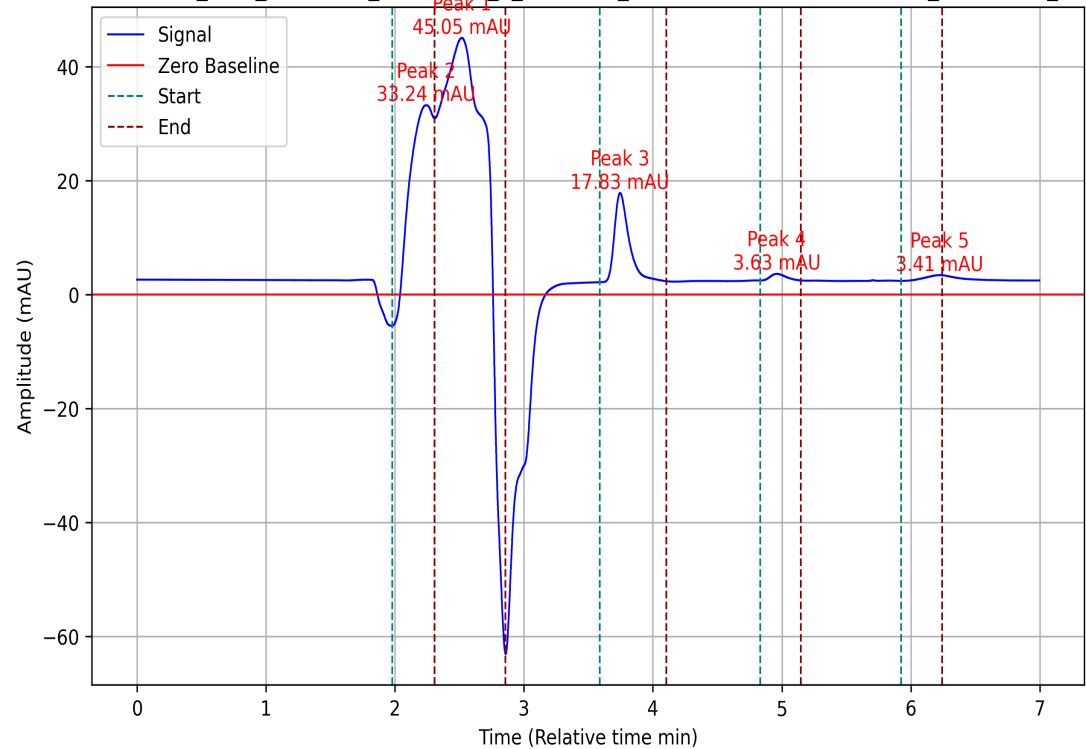


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
7	8	1	TE00003-4	955.592	2.51888	1.07231	45.055

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\8_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_210126.txt

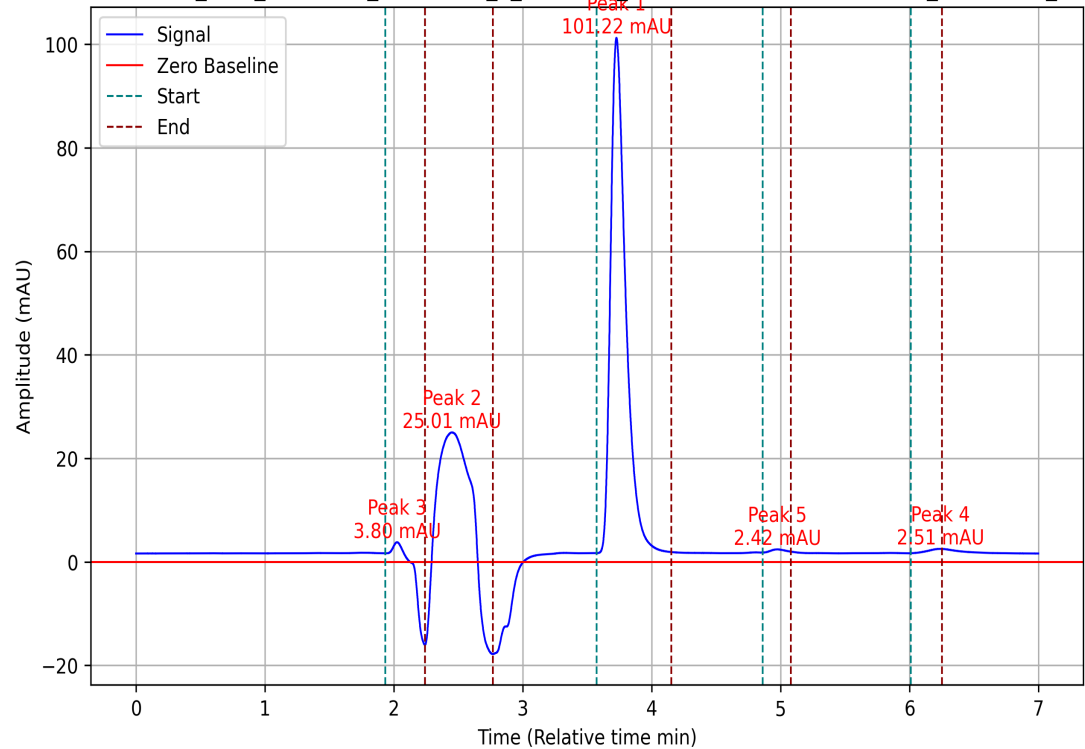


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
8	9	1	TE00003-5	872.074	3.72732	1.58973	101.22

Image for SAMPLE Inject ID: 1

HPLC Data: C:\raw_data_202602\9_26022301_1_ANALYZE_B4502842 - CETIRIZINE HCL_20260223_213744.txt

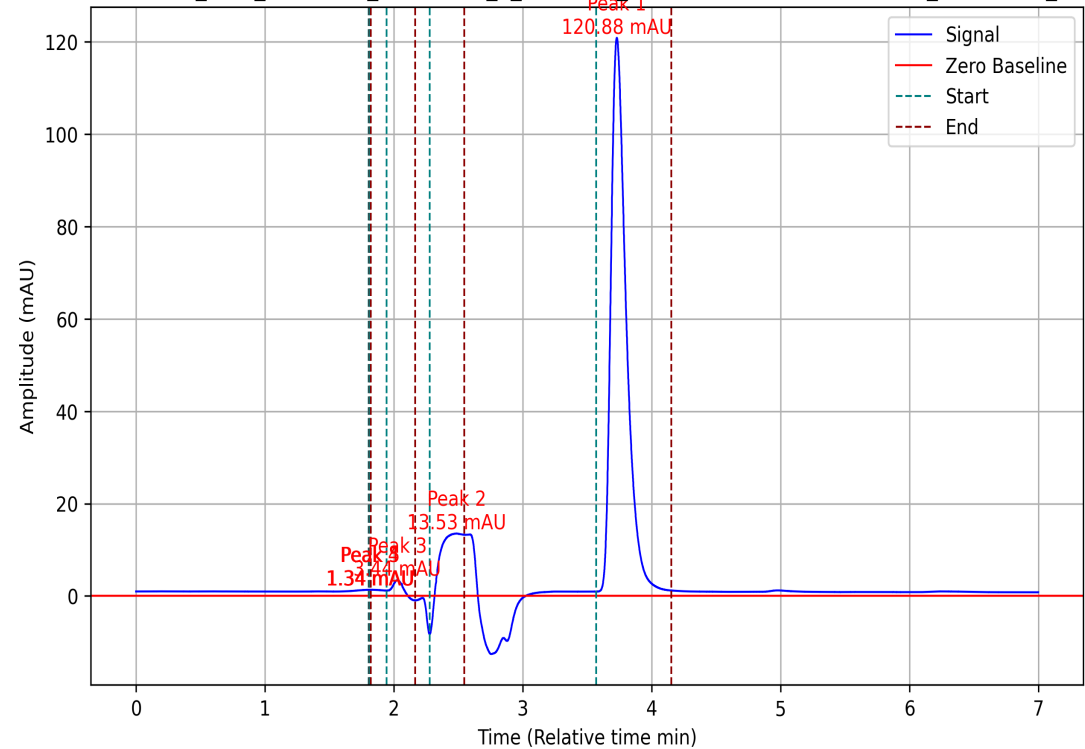

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING


Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
9	10	1	TE00003-6	1024.95	3.72893	1.57945	120.879

IMAGE DATA FOR BASELINE

Image for BASELINE Inject ID: 1

HPLC Data: C:\raw_data_202602\1_26022301_1_CLEANSE CHECKER_B4502842 - CETIRIZINE HCL_20260223_142526.txt

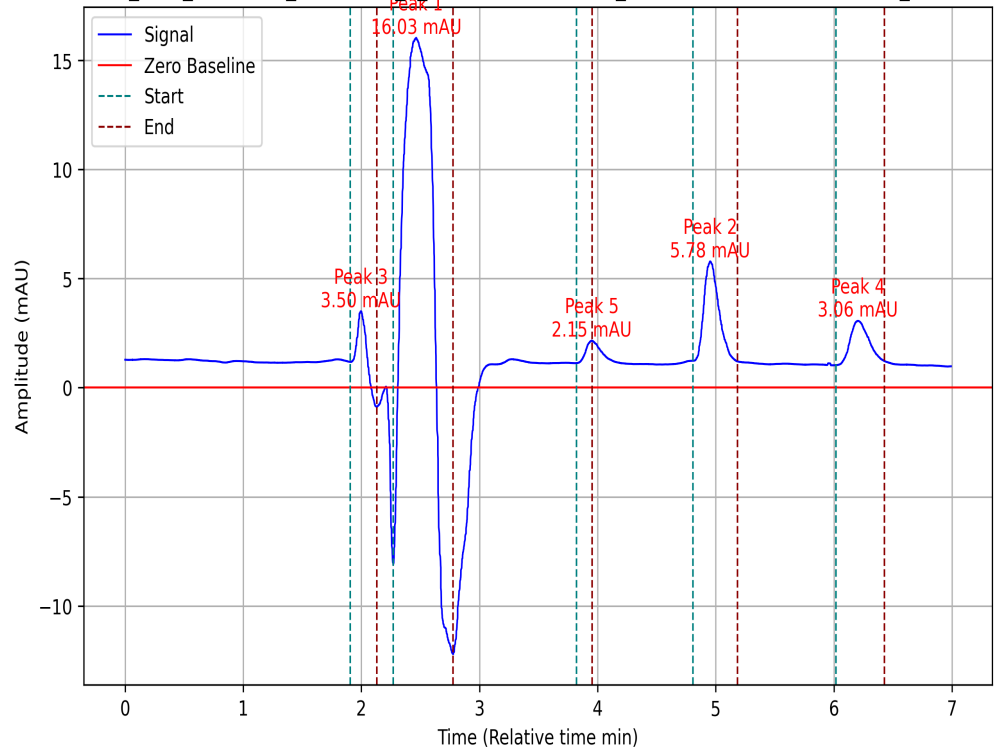


Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
1	2	1	TE00001-1	237.645	2.46422	1.05396	16.025
1	2	1	TE00001-1	67.5037	4.95365	1.29104	5.783
1	2	1	TE00001-1	20.8548	1.99585	0.943122	3.498
1	2	1	TE00001-1	48.1471	6.2029	1.10672	3.06
1	2	1	TE00001-1	12.8517	3.95117	0.51616	2.153

Image for DETECTOR CHECKER Inject ID: 1

HPLC Data: C:\raw_data_202602\10_26022301_1_DETECTOR CHECKER_B4502842 - CETIRIZINE HCL_20260223_214929.txt

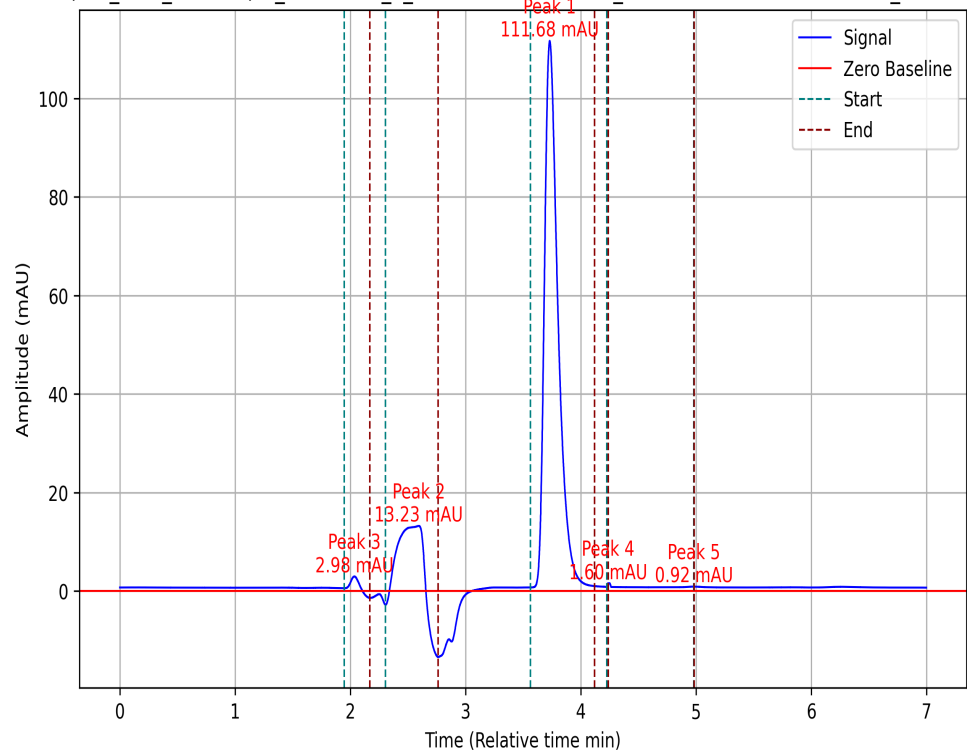

Company Name: PHAROS
Machine Name: FA250000001-FACTORY QC
Analysis ID: 26022301
Analysis Type: DISSOLUTION
Purpose: ANALYZE
Group Template ID: GT00001
Analysis Purpose: BATCH PRODUCTION
Batch Number: D6B631A
Product Name: OZEN 10 MG
Active Substance: B4502842 - CETIRIZINE HCL
Sample Origin Process: COATING

Result:

Order Number	Vial	Injection Number	Sample ID	Area	Retention Time (min)	Tailing Factor	Peak Height
10	4	1	TE00002-2	932.033	3.72928	1.5696	111.682
10	4	1	TE00002-2	191.306	2.59432	0.617663	13.235
10	4	1	TE00002-2	15.3047	2.03522	0.880759	2.976
10	4	1	TE00002-2	0.926144	4.23712	0.5	1.604
10	4	1	TE00002-2	0.095004	4.9826	0.5	0.915